



LMA® Unique (Silicone Cuff) Airway with Cuff Pilot Technology

The Single-Use, First-Generation LMA® Airway with a Silicone Cuff

A Versatile First-Generation Laryngeal Mask

The LMA® Unique (Silicone Cuff) Airway with Cuff Pilot Technology from Teleflex is a versatile, single-use, first-generation laryngeal mask with a medical-grade silicone cuff. Designed for patient comfort, the silicone cuff is soft and flexible, and conforms to the anatomy to create an effective oropharyngeal seal.^{1,2} The LMA® Unique (Silicone Cuff) Airway may be used for routine anesthetic procedures, for difficult airway situations, or for airway management during cardiopulmonary resuscitation. Its single-use design avoids the cleaning and sterilization costs associated with reusable devices,³ and may help to reduce the risk of cross-contamination.^{4,5}

Cuff Pilot Technology

The LMA® Unique (Silicone Cuff) Airway is available with Cuff Pilot Technology – an integrated, single-use cuff pressure indicator that constantly monitors cuff pressure, detecting changes resulting from fluctuations in temperature, nitrous oxide levels and movements within the airway. It provides at-a-glance feedback, highlighting changes that could affect patient safety.

Cuff Pilot Technology was developed to support clinicians in avoiding the known risks of cuff hyperinflation, which include sore throat, dysphagia, an increased risk of aspiration due to leakage around the cuff, and hypoglossal, lingual or recurrent laryngeal nerve palsies.^{6–10}

Benefits



The Clinician

Indicated for use in a wide range of clinical situations



Your Institution


Suited for areas where a reusable device is not practical, economical or desired



The Patient

Soft, medical-grade silicone cuff designed for patient comfort

LMA® Unique (Silicone Cuff) Airway with Cuff Pilot Technology

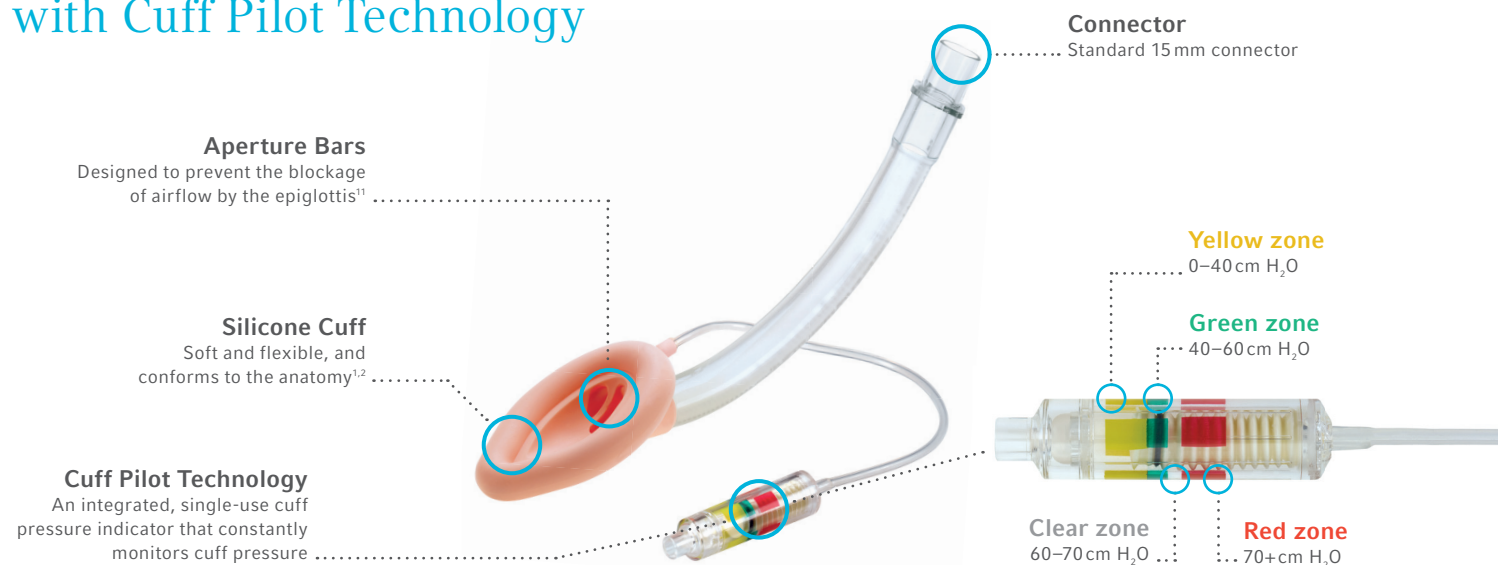

LMA® Unique (Silicone Cuff) Airway with Cuff Pilot Technology Fast Facts

Combines all of the features of the LMA® Unique Airway with the added benefits of a silicone cuff and integrated cuff pressure monitoring.^{1,2,12}

Silicone cuffs are better able to mold into shape, compared with PVC cuffs, and this may result in improved airway sealing characteristics.²

Supplied sterile for single use, and available with or without Cuff Pilot Technology in sizes.¹⁻⁶

LMA® Unique (Silicone Cuff) Airway with Cuff Pilot Technology*

ITEM NUMBER	MASK SIZE	PATIENT WEIGHT (KG)	MAXIMUM INTRACUFF PRESSURE (CM H ₂ O)
105200-000010	1	Up to 5	60
105200-000015	1.5	5–10	60
105200-000020	2	10–20	60
105200-000025	2.5	20–30	60
105200-000030	3	30–50	60
105200-000040	4	50–70	60
105200-000050	5	70–100	60
105200-000060	6	Over 100	60

* It is recommended that the cuff be inflated to a maximum of 60 cm H₂O intracuff pressure.



teleflex.com/LMA

References

- Eschertzhuber S, Brimacombe J, Hohliedier M, Keller C. *Anaesthesia*. 2009;64(1):79-83.
- Jagannathan N, Sohn LE, Sawardekar A, Gordon J, Langen KE, Anderson K. *Anaesthesia*. 2012;67(6):632-639.
- Soulias M, Martin L, Garnier N, Juniot A, Aho LS, Freysz M. *Ann Fr Anesth Reanim*. 2006;25(8):811-814.
- Miller DM, Youkhana I, Karunaratne WU, Pearce A. *Anaesthesia*. 2001;56(11):1069-1072.
- Greenwood J, Green N, Power G. *Anaesth Intensive Care*. 2006;34(3):343-346.
- van Zundert T, Brimacombe J. *Anaesthesiol Intensive Ther*. 2012;44(2):63-70.
- Bick E, Bailes I, Patel A, Brain AI. *Anaesthesia*. 2014;69(12):1304-1308.
- Burgard G, Mollhoff T, Prien T. *J Clin Anesth*. 1996;8(3):198-201.
- Chantzara G, Stroumpoulis K, Alexandrou N, Kokkinos L, Iacovidou N, Xanthos T. *Minerva Anesthesiol*. 2014;80(5):547-555.
- Seet E, Yousaf F, Gupta S, Subramanyam R, Wong DT, Chung F. *Anesthesiology*. 2010;112(3):652-657.
- Benumof JL. *Can J Anaesth*. 2003;50(9):968.
- Martin DP, Bhalla T, Thung A, Tobias JD. *Int J Pediatr Otorhinolaryngol*. 2013;77(1):76-78.

Teleflex, the Teleflex logo, Cuff Pilot, LMA and LMA Unique are trademarks or registered trademarks of Teleflex Incorporated or its affiliates, in the U.S. and/or other countries. Information in this document is not a substitute for the product Instructions for Use. The products in this document may not be available in all countries. Please contact your local representative. All data current at time of printing (03/2019). Subject to technical changes without further notice. © 2019 Teleflex Incorporated. All rights reserved. MCI-2019-0801 · EN · REV 0 · PDF

Teleflex

Distributed by:
Teleflex Headquarters International, Ireland · Teleflex Medical Europe Ltd. · IDA Business & Technology Park
Dublin Road · Athlone · Co Westmeath · Tel. +353 (0)9 06 46 08 00 · Fax +353 (0)14 37 07 73 · orders.intl@teleflex.com
United Kingdom Tel. +44 (0)14 94 53 27 61 · info.uk@teleflex.com
South Africa Tel. +27 (0)11 807 4887 · assist.africa@teleflex.com